

SEPARATE TYPE ELECTROMAGNETIC FLOWMETER

DATA SHEET

FMB1, 2/ FMC

The electromagnetic flowmeter is an instrument to measure the volumetric flow rate of liquid simply by applying a magnetic field from the outside utilizing the fact that an electric conductor which crosses a magnetic field at a certain velocity causes voltage to be induced in proportion to the velocity, which is known as Faraday's law.

This flowmeter is designed with the latest electronics technology and magnetic/electric field analyzing technology, realizing a compact and light-weight structure and measurement with high accuracy.

FEATURES

1. High accuracy

The adoption of the optimum magnetic field design using the 3-dimensional finite element method has minimized the effects of flow velocity profile and materials of adjacent piping. At flow velocity of more than 1m/sFS, the measurement accuracy is as high as $\pm 0.5\%$ of indicated value when the flow is above 20%FS.

2. Wide range

Measurement range: 0 to 0.3 ... 15m/sec in flow velocity

3. High-reliability structure

The sensor terminal box is a sealed 2 - chamber structure, practically free from dew condensation and sudden submergence. The adoption of stainless housing assures excellent anti-environment efficiency.

4. Easy-to-see display


LCD with back-light allows easy check of display even in a dark place. Instantaneous flow and integral volumetric flow are displayed at the same time.

5. Free power supply

The flowmeter operates on power supply 100 to 240V AC, 50/60 Hz, eliminating the need for selection of power voltage.

6. Application of international standards

The overall length of flange type flowmeter conforms with ISO draft standards. (Meter size : 6A-200A)

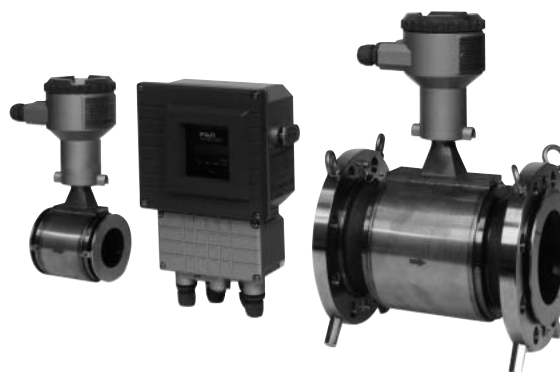

• Mounting method :

Mounted via flange insertion type on opposite side (wafer type)(with Guide rings)
... 2.5 to 200A

Note 1) Guide ring : A ring-shaped guide used for centering the sensor when a wafer type is mounted on the piping.
or flange mounting
... 6 to 300A

Note 2) Flange with meter size 2.5A or 6A can be used for 15A.

• Liquid pressure :

-100 to 2000kPa or flange operating

• Meter size and measurement range :

Measuring range is equivalent to flow velocity 0.3 to 15m/s.

Meter size	Min.measurement range [m ³ /h]	Max. measurement range [m ³ /h]
2.5A Note 3)	0 to 0.00531	0 to 0.265
6A	0 to 0.0306	0 to 1.52
15A	0 to 0.191	0 to 9.54
25A	0 to 0.531	0 to 26.5
40A	0 to 1.36	0 to 67.8
50A	0 to 2.13	0 to 106
80A	0 to 5.43	0 to 271
100A	0 to 8.49	0 to 424
150A	0 to 19.1	0 to 954
200A	0 to 34.0	0 to 1696
250A	0 to 53.1	0 to 2650
300A	0 to 76.4	0 to 3817

Note) Meter size 2.5A: Wafer type only

SPECIFICATIONS

Sensor (Type : FMB)

• Measurement item :


General-use industrial water, tap-water, sewage, waste water, chemicals slurry, and other liquids with conductivity of more than 3 μ S/cm

• Structure :

Wafer type or flange type

• **Liquid temperature :**

- 10 to +120°C (Tefron lining)
- 10 to +50°C (Polyurethane lining)

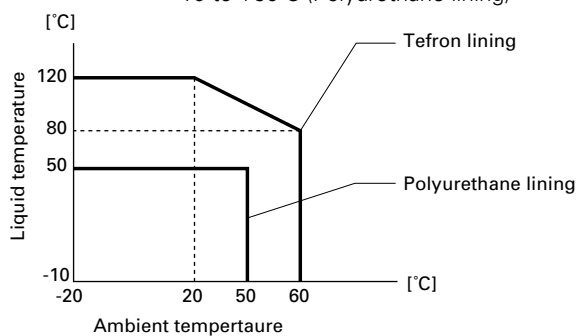

Ambient temperature-liquid temperature allowable range

• **Material :**

	Lining	Tefron(PFA, TFE)	Polyurethane
Parts in contact with liquid (Note 1)	Electrode	SUS316L Hasteroy C Titanium Tantalum Platinum iridium	SUS316L
	Earth ring	SUS316 Not L Hasteroy C Titanium Tantalum	SUS316 Not L
	Housing case	SUS304	
	Flange (Note 2)	SUS304 or carbon steel	
	Terminal box case	Aluminum alloy	

Note 1) Materials of parts in contact with liquid should be selected in consideration of erosion due to measuring liquid. Refer to the table of material selection on the attached sheet.

Note 2) Flange type only

• **Piping connection port :**

G $\frac{1}{2}$, NPT $\frac{1}{2}$, Pg 13,5, M20x5

• **Painting :**

Terminal box case; Polyurethane corrosion-resistant painting (Silver)

Cover; Polyurethane corrosion-resistant painting (Blue)

Flange; SUS304 type is unpainting.
Carbon steel type is polyurethane corrosion-resistant painting (Silver).

• **Structure :**

JIS C 0920 immersion-proof (IP67)

• **Grounding :**

D-class grounding (100Ω or less)

Converter (Type FMC)

• **Mounting method :**

Pipe or wall mounting

• **Exciting system :**

Square low-frequency exciting

• **Input/output signal :**

Current output; 4 to 20mA DC
Load resistance 0 to 1KΩ
Pulse output; open-collector
Capacity; DC30V, 0.2A or less
ON voltage; 0.6V or less
0.0001 to 1000P/s
Status output; open-collector
Capacity; DC30V, 0.2A or less
ON voltage; 2V or less
Status input; no-voltage contact
Note) Status signal input or output, either one, can be

• **Pulse output :** Integrated pulses are outputted by setting integral constant. Pulse width 0.5 to 80ms

• **Span setting :**

Flow FS can be set by setting flow unit and flow value. Flow velocity can also be set.
Display cubic volume, length; m³, L, mL, m

Display time unit ; /d, /h, /min, /s

• **Multi-range :** Automatic 2-range selection in 2-range select mode. External 2-range selection with status input is possible.

• **Flow direction change :**

Flow direction can be reversed in flow direction mode.

• **Flow display :**

Real time flow display, % display or user unit display is possible in 7 codes, max.

• **Integration display :**

Integrated volumetric flow can be displayed by setting the unit of cubic volume. Displayed cubic volume; m³, L, mL

• **Fault diagnosis function :**

Various fault can be diagnosed by hardware check and process check.

• **Zero point adjustment :**

Zero point is automatically calibrated with one-push operation.

• **Output low cut :**

0 to 10% FS

Momentary output can be cut to 0% at flow rate below the set cutoff point.

• **Integration low cut :**

0 to 10% FS

Integration of display and output are prevented at flow rate below the set cutoff point.

• **0% signal lock :**

Display and output can be locked to 0% with status input.

• **Slurry noise cut :**

0 to 10% FS, 0 to 60 sec

Slurry noise (spike noise) can be cut by setting rate limit.

• **Empty detection :**

Absence of liquid is detected and status signal is outputted.

• **Flow switch :**

-10 to 110% FS

Status signal is outputted by setting high/low limit flow.

• **Dumping time constant :**

1 to 200 sec

• **Converter case :**

Aluminum alloy

• **Arrester :**

Built-in power supply arrester and current output arrester

• **Wiring connection port :**

G $\frac{1}{2}$, NPT $\frac{1}{2}$, Pg 13,5, M20 x 1,5

• **Painting :**

Body case, terminal box case or cover; Polyurethane corrosion-resistant painting (Silver)

Body cover;

Polyurethane corrosion-resistant painting (Blue)

• **Structure :**

JIS C 0920 immersion-proof (IP67)


• **Grounding :**

D-class grounding (100Ω or less)

• **Mass :**

3.5kg

- Length of special signal cable:
150m or less (see diagram below)

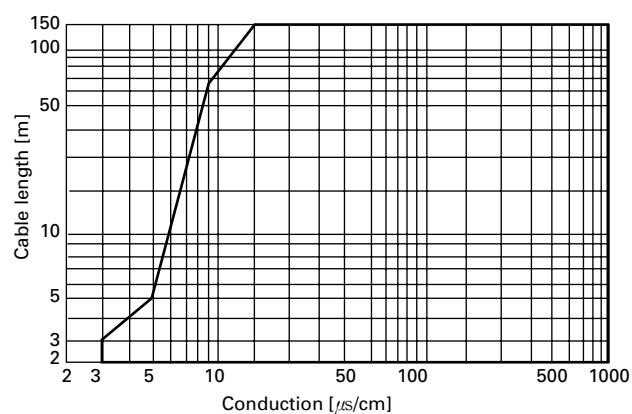

Allowable length of special signal cable

OTHER SPECIFICATIONS

When replacing Fuji's former type sensors, flanges with short pipe are available. For details, contact our office.

For specifications of special water-proof type, etc., contact our office.

Standard performance


- Accuracy rating :

Meter size	2.5A to 15A	25A to 200A
FS flow velocity 1m/s or more	Flow velocity $\geq 50\%FS$: $\pm 0.5\%$ of rate Flow velocity $< 50\%FS$: $\pm 0.25\%$ FS	Flow velocity $\geq 20\%FS$: $\pm 0.5\%$ of rate Flow velocity $< 20\%FS$: $\pm 0.1\%$ FS
FS flow velocity 0.3m/s or more less than 1m/s	$\pm 0.5\%$ FS	Flow velocity $\geq 50\%FS$: $\pm 0.5\%$ of rate Flow velocity $< 50\%FS$: $\pm 0.25\%$ FS

- Power consumption :
12W or less
- Operating condition :
Ambient temperature;
-20 to 60°C (Teflon lining sensor)
-20 to 50°C (Urethane lining sensor)
-20 to 60°C (converter)
Ambient humidity; 95% RH or less
Power voltage; 100 to 240V AC $\pm 10\%$
Power frequency; 50/60Hz

Length of straight pipe

The length of the up-stream/down-stream straight pipe of the detector should be long enough to ensure accurate measurements. See below.

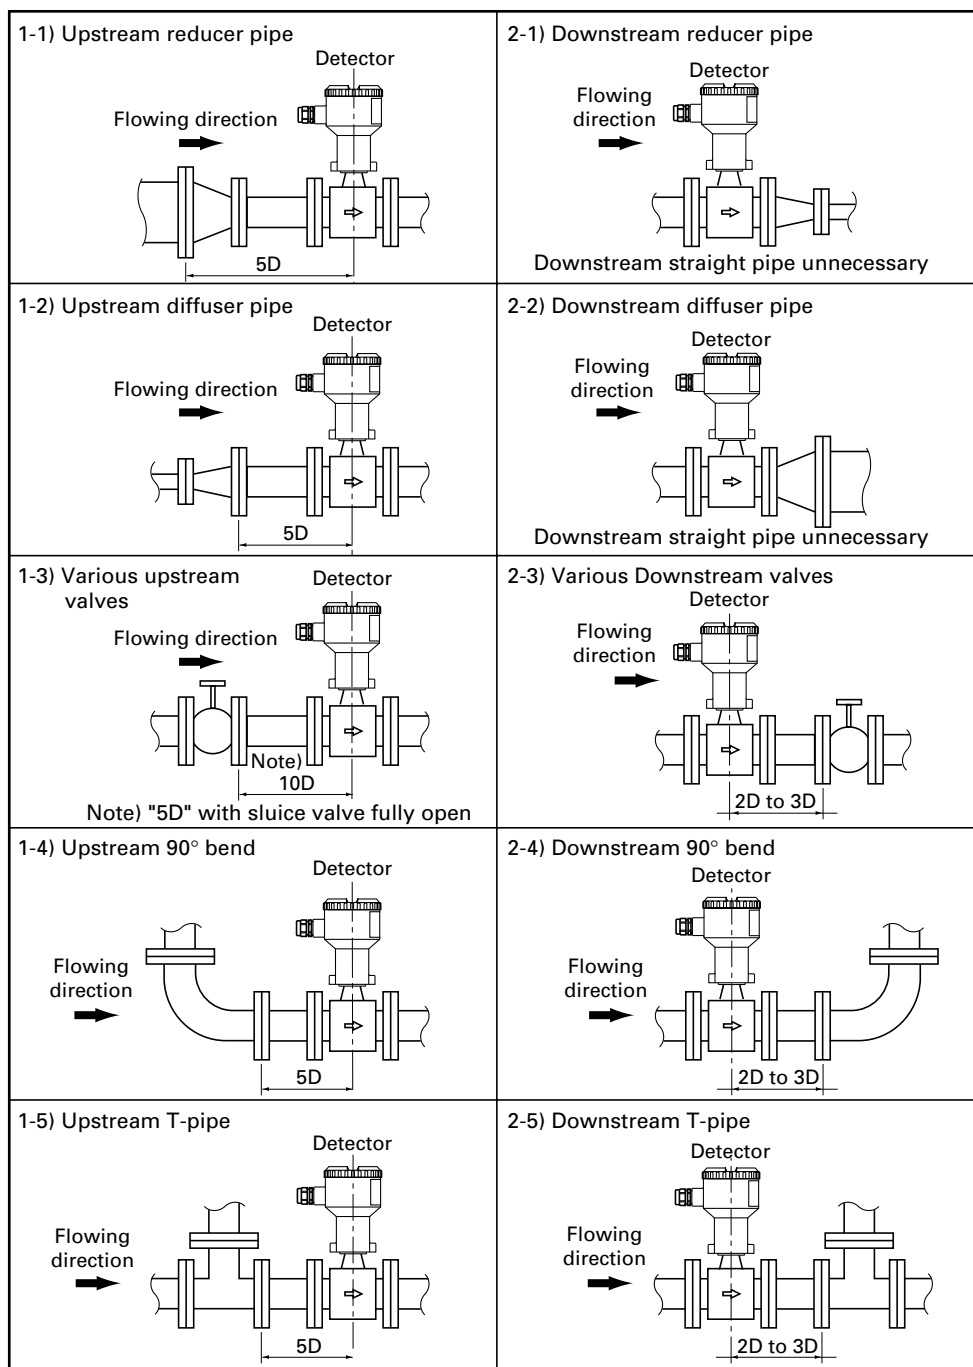

Minimum length of straight pipe between upstream/downstream joints and flowmeter

Note 1) $L = a \text{ multiple of diameter } D \text{ of measuring pipe.}$


Note 2) Do not put any objects, which affect magnetic field, electromotive force and flow profile, in the measuring pipe.

Note 3) Use a straight pipe (2D to 3D) on the downstream side, if the drift to the upstream side is affected by installing valves, etc.

Mounting posture


The detector can be installed vertically, horizontally, or at other angle. When installing, be sure to observe the following points.

- ① The measuring pipe should always fill with fluid which flows in the piping.

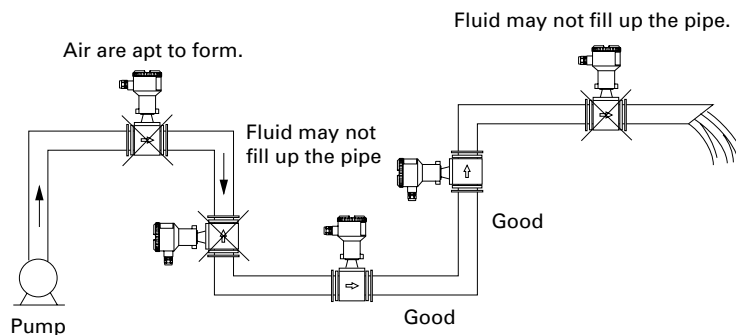


Example of mounting posture

- ② The electrode should be at a level with the ground and should always keep contact with fluid. (If the electrode is vertical to the ground, air bubbles appear on the fluid and hence correct measurements cannot be expected; also, the low part of the electrode is easily contaminated with deposits.)

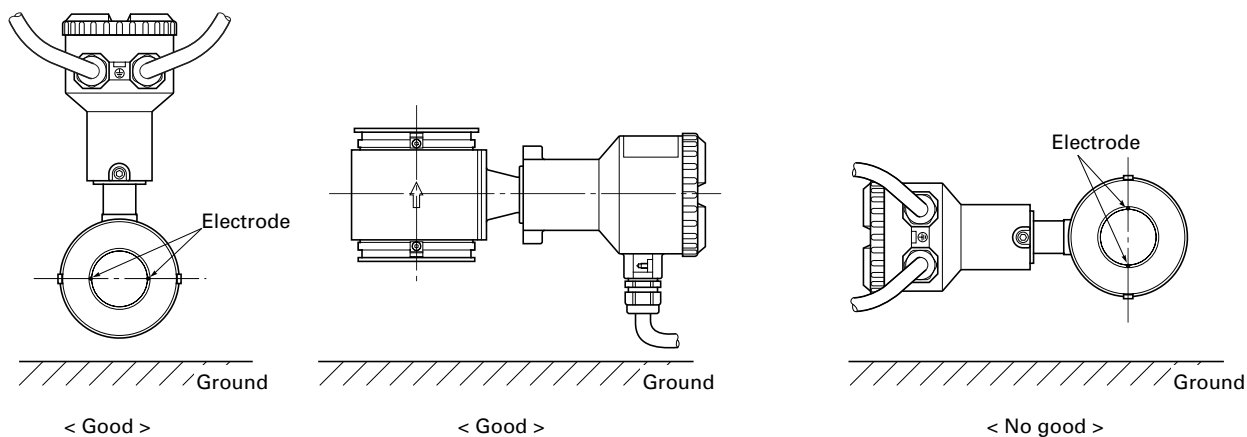


Electrode mounting position

- ③ Use of a bypass valve will provide easy zero adjustment and maintenance. Install a bypass line so that fluid flow is not interrupted. A bypass line installed as illustrated in following figure (a) and (b) allows the inside of the pipe to be washed and cleaned without removing the flowmeter.

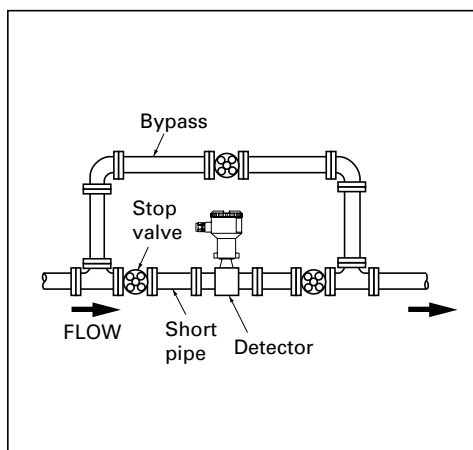

(a) Horizontal bypass line

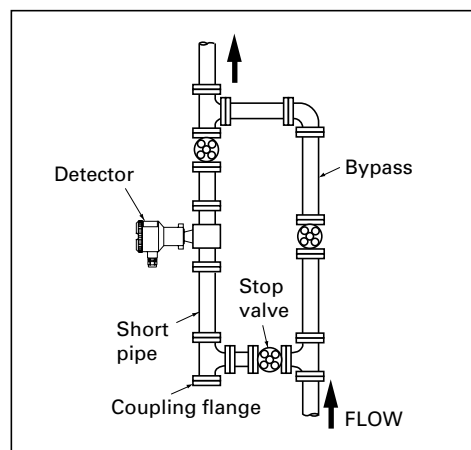

(b) Vertical bypass line

Material selection table

The following table indicates examples of recommended materials, contacting with liquid, to be used with the typical liquids measured with electromagnetic flowmeter. Evaluation of those materials has been conducted according to various documents and experience in actual use.

1. Characteristics of lining materials

[◎ : Excellent, ○ : Very good, △ : Good, × : No good]

Material	Abrasion resistance	Heat resistance	Corrosion resistance	Adhesion resistance	Remarks
Teflon PFA	×	◎	◎	◎	Ideal for the use with corrosive or adhesive fluids. Not suitable for abrasive fluid (such as slurry.) * Pay attention to permeability of TFE. Note that TFE is not suitable for use with high-temperature + negative pressure fluid.
Teflon TFE	×	◎	◎	◎	
Poly-urethane	○	×	×	△	Has inferior heat resistance or corrosion resistance. Best for slurry or the like with no corrosive properties.

2. Material selection table of electrode/earth ring

Material	Measurable liquid	Unmeasurable liquid
SUS316	Water and waste water, weak acid, weak alkali Example: 25% acetic acid or less, hydroiodic acid, butyric acid, aqueous ammonia or alike	Inorganic acid, organic acid, chloride or alike
Hastelloy C-276 or equivalent	Suitable for intermediate oxidation and reduction and can be used for various fields. Example: Sea water, formic acid, acetic acid, aqueous ammonia, normal-temperature (lower than 40°C) nitric acid, hydrochloric acid and sulfuric acid or alike	Chloride, high-temperature strong acids (nitric acid, hydrochloric acid, sulfuric acid), high temperature (higher than 40°C) or high concentration (more than 40%) ferric chloride or alike
Titanium	Resistant to sea water, most oxidative acids, chloride, sulfide and alkali. Example: Sea water, saline water, aqueous ammonia, chlorine water, polyelectrolyte, acetic acid, ferric chloride or alike	Reductive acids such as hydrochloric acid, sulfuric acid, phosphoric acid, oxalic acid
Tantalum	Resistant to most chemicals. (particularly, strong acids) Example: Hydrochloric acid, sulfuric acid, nitric acid, aqua regia, ferric chloride, hypochlorous acid, sodium hypochlorite, PAC (Polyaluminum chloride) or alike	Sodium hydroxide, potassium hydroxide, hydrofluoric acid, fuming sulfuric acid or alike
Platinum-iridium (Pt-Ir)	Resistant to almost chemicals.	Aqua regia

CODE SYMBOLS

Separate type electromagnetic flowmeter sensor (wafer type)

1	2	3	4	5	6	7	8	9	10	11	12	13	14	
F	M	B	1				1		0		0			
														Description
														Meter size (5th code)
														2.5A
														6A
														15A
														25A
														40A
														50A
														80A
														100A
														150A
														200A
														Lining material (6th code)
														PFA mold Tefron
														Polyurethane rubber
														(7th & 9th code; W only)
														Note) Polyurethane rubber with less than 15A of meter size cannot be used.
														Earth ring material (7th code)
														SUS316
														Hasteroy C
														Titanium
														Tantalum
														Electrode material (9th code)
														SUS316L
														Hasteroy C
														Titanium
														Tantalum
														Platinum iridium
														Flange (10th code)
														None
														Guide ring (11th code)
														For JIS 10K
														For JIS 200K
														For JIS 75M (inside diameter of less than 50A cannot be used)
														For ANSI 150LB
														For ANSI 300LB
														For DIN/PN 16K
														For DIN/PN 40K
														Wiring connection port size (12th code)
														G1/2(PF1/2) female screw with water-proof gland
														G1/2(PF1/2) female screw with union and water-proof gland
														NPT1/2 female screw
														Pg 13.5 female screw
														M20 ×1.5 female screw
														Application (13th code)
														General type
														Optional specifications (14th code)
														None
														Stainless tag plate

Separate type electromagnetic flowmeter sensor (flange type)


1	2	3	4	5	6	7	8	9	10	11	12	13	14	Description
F	M	B	2				1	0	0	0				
A														Meter size (5th code)
C														6A Note
D														15A
T														25A
E														40A
F														50A
G														80A
H														100A
J														150A
K														200A
L														250A
														300A
														Note) Flange size for meter size 6A is 15A or 1/2B.
P														Lining material (6th code)
T														PFA mold Tefron Note 1
U														TFE Tefron Note 2
														Polyurethane rubber Note 3
														(7th & 9th codes: W only)
														Note 1) PFA 6A to 200A
														Note 2) TFE 250A, 300A
														Note 3) Polyurethane rubber with less than 15A of meter size cannot be used.
W														Earth ring material (7th code)
H														SUS316
C														Hasteroy C
T														Titanium
														Tantalum
W														Electrode material (9th code)
H														SUS316L
C														Hasteroy C
T														Titanium
P														Tantalum
														Platinum iridium
1														Flange standard Flange material
2														JIS 10K SUS304
4														JIS 20K SUS304
5														JIS 75M SUS304 Note 2
6														ANSI 150LB SUS304
7														ANSI 300LB SUS304
8														DIN PN16 SUS304
A														DIN PN40 SUS304 Note 1
B														JIS 10K Carbon steel
D														JIS 20K Carbon steel Note 3
E														JIS 75M Carbon steel Note 2
F														ANSI 150LB Carbon steel
G														ANSI 300LB Carbon steel
H														DIN PN16 Carbon steel
														DIN PN40 Carbon steel Note 1
														Note 1) Mater size 100A or more cannot be used.
														Note 2) Mater size 50A or less cannot be used.
														Note 3) Mater size 250A or 300A can be selected only for A, B and D.
0														Guide ring (11th code)
														None
A														Wiring connection port size (12th code)
B														G $\frac{1}{2}$ (PF $\frac{1}{2}$) female screw with
C														water-proof gland G $\frac{1}{2}$ (PF $\frac{1}{2}$) female screw with
D														union and water-proof gland
E														NPT $\frac{1}{2}$ female screw
														Pg 13.5 female screw
														M20×1.5 female screw
1														Direction of indicator (13th code)
2														Horizontal mounting
														Vertical mounting
Y														Optional specifications (14th code)
A														None
														Stainless tag plate

Converter (separate type)


1	2	3	4	5	6	7	8	9	10	11	12	13	Description
F	M	C	1	N			1	-					Application (4th code)
			1										General use
				N									Power supply (5th code)
													AC100 to 240V 50/60Hz
													Mounting method (6th code)
					A								Pipe mounting
					B								Wall mounting
													Wiring connection port size (7th code)
						Y							G1/2(PF1/2) female screw
						A							G1/2(PF1/2) female screw with water-proof gland
						B							G1/2(PF1/2) female screw with union and water-proof gland
						C							NPT1/2 female screw
						D							Pg 13.5 female screw
						E							M20×1.5 female screw
													Optional specifications (9th code)
							Y						None
							A						Parameter setting
													Note) When parameter setting function is used, specify parameters in parameter designation tables 1 and 2.
													Cable end treatment (10th code)
							Y						Without cable end treatment
							A						With cable end treatment
													Cable length (11 to 13th code)
								0	0	0			0
								0	0	5			5m
								0	1	0			10m
								0	1	5			15m
								0	2	0			20m
								0	2	5			25m
								0	3	0			30m
								0	3	5			35m
								0	4	0			40m
								0	5	0			50m
								0	6	0			60m
								0	7	0			70m
								0	8	0			80m
								0	9	0			90m
								1	0	0			100m
								1	1	0			110m
								1	2	0			120m
								1	3	0			130m
								1	4	0			140m
								1	5	0			150m

OUTLINE DIAGRAM (Unit: mm)

(Wafer type sensor)

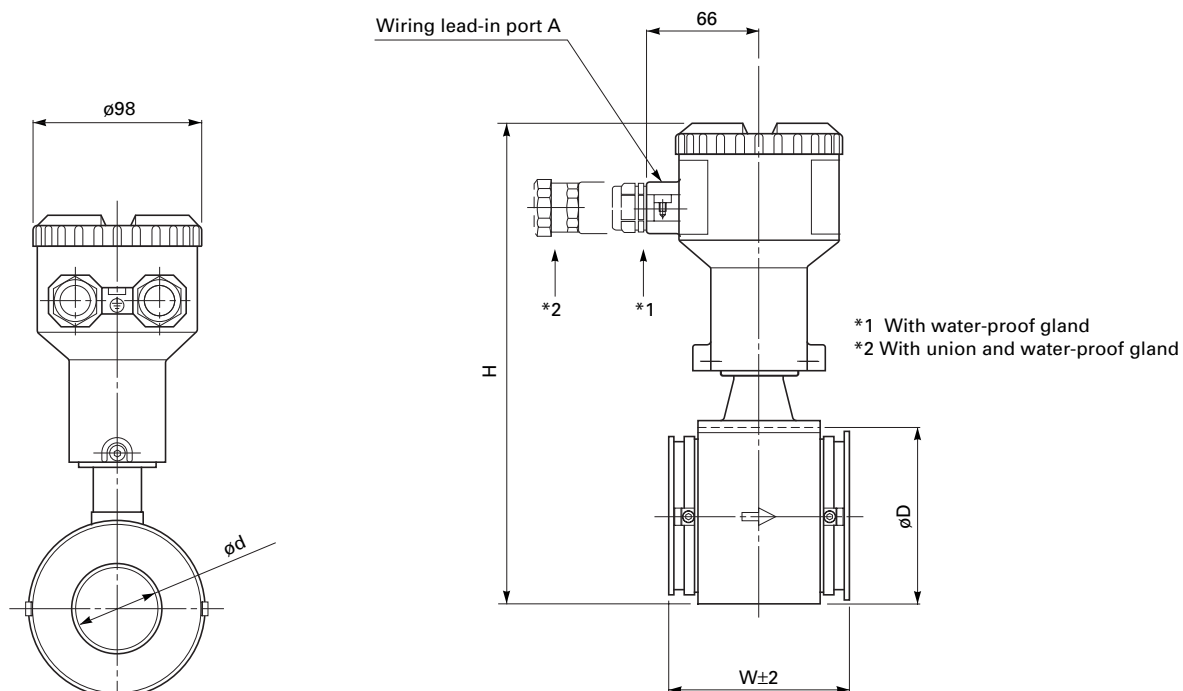

Note) When earth ring material is tantalum, W is shortened by 4mm.

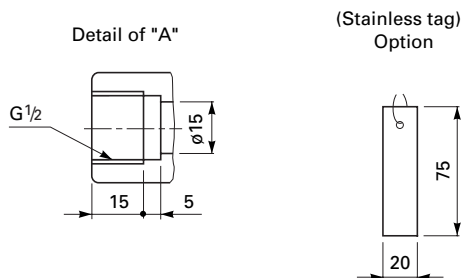


Mater size	W	ød	øD	H	Mass (Kg)
2.5A	85	2.5	50	231	2
6A	85	6	50	231	2
15A	85	12	50	231	2
25A	93	22.6	68	249	2.5
40A	100	35.6	86	267	3.5
50A	105	47.8	96	277	4
80A	150	72.3	125	306	7.5
100A	160	97.6	160	351	10
150A	190	150	211	402	14.5
200A	205	200	271	462	24.5

M	L1	L2
G 1/2	13.5	18.5
NPT 1/2	16	21
Pg13.5	10.5	15
M20 × 1	16	21

OUTLINE DIAGRAM (Unit: mm)

(Flange type sensor)

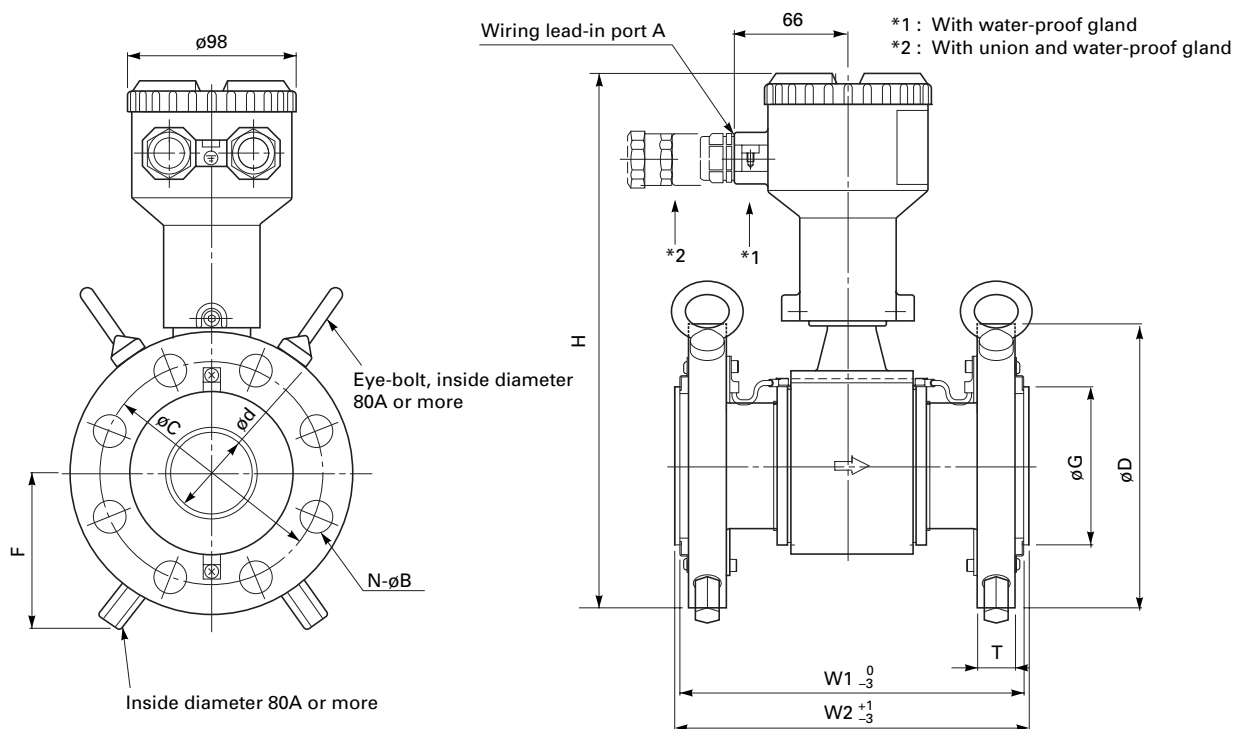


Note) When earth ring material is tantalum, W2 is shortened by 4mm.


JIS Flange

Meter size	6A(Note1)	15A	25A	40A	50A	80A	100A	150A	200A
W1	200	200	200	200	200	200	250	300	350
W2	206	206	206	206	206	206	256	306	356
JIS 10K flange	ϕD	95	95	125	140	155	185	210	280
	ϕC	70	70	90	105	120	150	175	240
	N- ϕB	4-15	4-15	4-19	4-19	4-19	8-19	8-19	8-23
	T	12	12	14	16	16	18	18	22
	ϕG	46	46	66	82	92	121	152	202
	ϕd	6	12	22.6	35.6	47.8	72.3	97.6	150
	H	253	253	277	294	306	336	376	436
	F	-	-	-	-	-	102	112	144
JIS 20K flange	Mass (Kg)	3.5	3.5	5.5	7.5	8.5	14.5	18.5	32.5
	ϕD	95	95	125	140	155	200	225	305
	ϕC	70	70	90	105	120	160	185	260
	N- ϕB	4-15	4-15	4-19	4-19	8-19	8-23	8-23	12-25
	T	14	14	16	18	18	22	24	28
	ϕG	46	46	66	82	92	121	152	202
	ϕd	6	12	22.6	35.6	47.8	72.3	97.6	150
	H	253	253	277	294	306	343	383	449
JIS 75M flange	F	-	-	-	-	-	108	118	160
	Mass (Kg)	3.5	3.5	6	8	8.5	16.5	21.5	39
	ϕD	-	-	-	-	-	211	238	290
	ϕC	-	-	-	-	-	168	195	247
	N- ϕB	-	-	-	-	-	4-19	4-19	6-19
	T	-	-	-	-	-	18	18	22
	ϕG	-	-	-	-	-	121	152	202
	ϕd	-	-	-	-	-	72.3	97.6	150
	H	-	-	-	-	-	349	390	441
	F	-	-	-	-	-	113	124	163
	Mass (Kg)	-	-	-	-	-	17	21.5	34.5
		-	-	-	-	-			52

Note 1 : For meter size 6A, use flange JIS 15A.

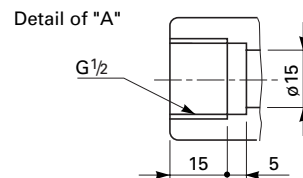

(Stainless tag)
Option



M	L1	L2
G $\frac{1}{2}$	13.5	18.5
NPT $\frac{1}{2}$	16	21
Pg13.5	10.5	15
M20 \times 1.5	16	21

ANSI flange

Meter size	$\frac{1}{4}$ B (Note2)	$\frac{1}{2}$ B	1B	$1\frac{1}{2}$ B	2B	3B	4B	6B	8B
W1	200	200	200	200	200	200	250	300	350
W2	206	206	206	206	206	206	256	306	356
ANSI 150LB flange	øD	89	89	108	127	152	191	229	279
	øC	60.3	60.3	79.4	98.4	120.6	152.4	190.5	241.3
	N-øB	4-16	4-16	4-16	4-16	4-20	4-20	8-20	8-23
	T	11.5	11.5	14.5	17.5	19.5	24	24	25.5
	øG	46	46	66	82	92	121	152	202
	ød	6	12	22.6	35.6	47.8	72.3	97.6	150
	H	250	250	269	287	305	339	385	436
	F	—	—	—	—	—	104	120	144
	Mass (Kg)	3	3	5	7	9	17	22.5	33.5
ANSI 300LB flange	øD	95	95	124	156	165	210	254	318
	øC	66.7	66.7	88.9	114.3	127	168.3	200	269.9
	N-øB	4-16	4-16	4-20	4-23	8-20	8-23	8-23	12-23
	T	14.5	14.5	17.5	21	22.5	29	32	37
	øG	46	46	66	82	92	121	152	202
	ød	6	12	22.6	35.6	47.8	72.3	97.6	150
	H	253	253	277	302	311	348	398	455
	F	—	—	—	—	—	112	130	165
	Mass (Kg)	3.5	3.5	6	9.5	10	20	30	48.5

Note 2 : For meter size 1/4B, use flange ANSI 1/2B.

DIN flange


Meter size	6A (Note3)	15A	25A	40A	50A	80A	100A	150A	200A
W1	200	200	200	200	200	200	250	300	350
W2	206	206	206	206	206	206	256	306	356
DIN PN16 flange	øD	95	95	115	150	165	200	220	285
	øC	65	65	85	110	125	160	180	240
	N-øB	4-14	4-14	4-14	4-18	4-18	8-18	8-18	8-22
	T	16	16	18	18	20	20	20	22
	øG	46	46	66	82	92	121	152	202
	ød	6	12	22.6	35.6	47.8	72.3	97.6	150
	H	253	253	272	299	311	343	381	439
	F	—	—	—	—	—	108	116	151
	Mass (Kg)	4	4	6	8.5	10	16.5	20	33
DIN PN40 flange	øD	95	95	115	150	165	200	—	—
	øC	65	65	85	110	125	160	—	—
	N-øB	4-14	4-14	4-14	4-18	4-18	8-18	—	—
	T	16	16	18	18	20	24	—	—
	øG	46	46	66	82	92	121	—	—
	ød	6	12	22.6	35.6	47.8	72.3	—	—
	H	253	253	272	299	311	343	—	—
	F	—	—	—	—	—	108	—	—
	Mass (Kg)	4	4	5.5	8.5	10	17.5	—	—

Note 3 : For meter size 6A, use flange DIN 15A.

OUTLINE DIAGRAM (Unit: mm)


*1 : With water-proof gland

*2 : For plica tube PV-5#17 with union and water-proof gland

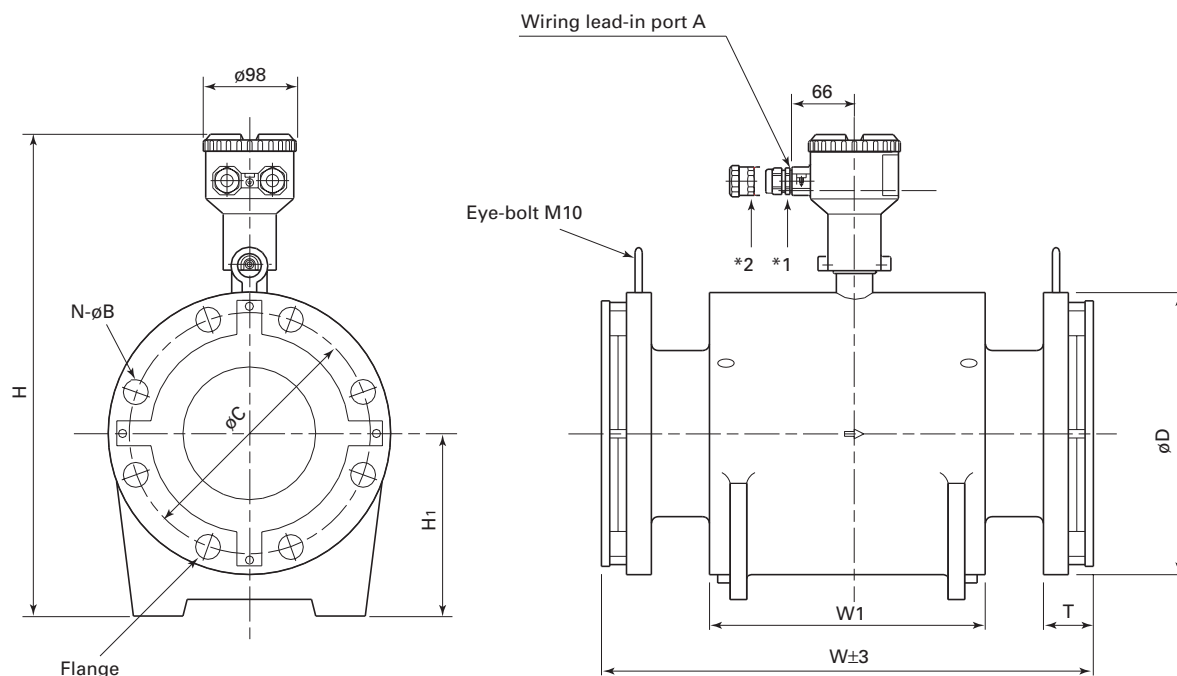

Detail of "A"

<Stainless tag> Option

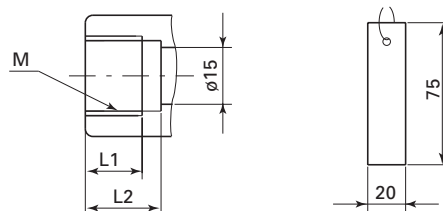


Meter size		250 A	300 A
W		595	595
W1		320	360
H		548	603
H1		220	250
JIS 10K Flange	ϕD	400	445
	ϕC	355	400
	N- ϕB	12-25	16-25
	T	36	38
	Mass (Kg)	95	113
JIS 20K Flange	ϕD	430	480
	ϕC	380	430
	N- ϕB	12-27	16-27
	T	46	48
	Mass (Kg)	98	118
JIS 75M Flange	ϕD	410	464
	ϕC	360	414
	N- ϕB	8-23	10-23
	T	36	38
	Mass (Kg)	95	113


M	L1	L2
G 1/2	13.5	18.5
NPT 1/2	16	21
Pg13.5	10.5	15
M20 \times 1.5	16	21


OUTLINE DIAGRAM (Unit: mm)

(Pipe mount type converter)

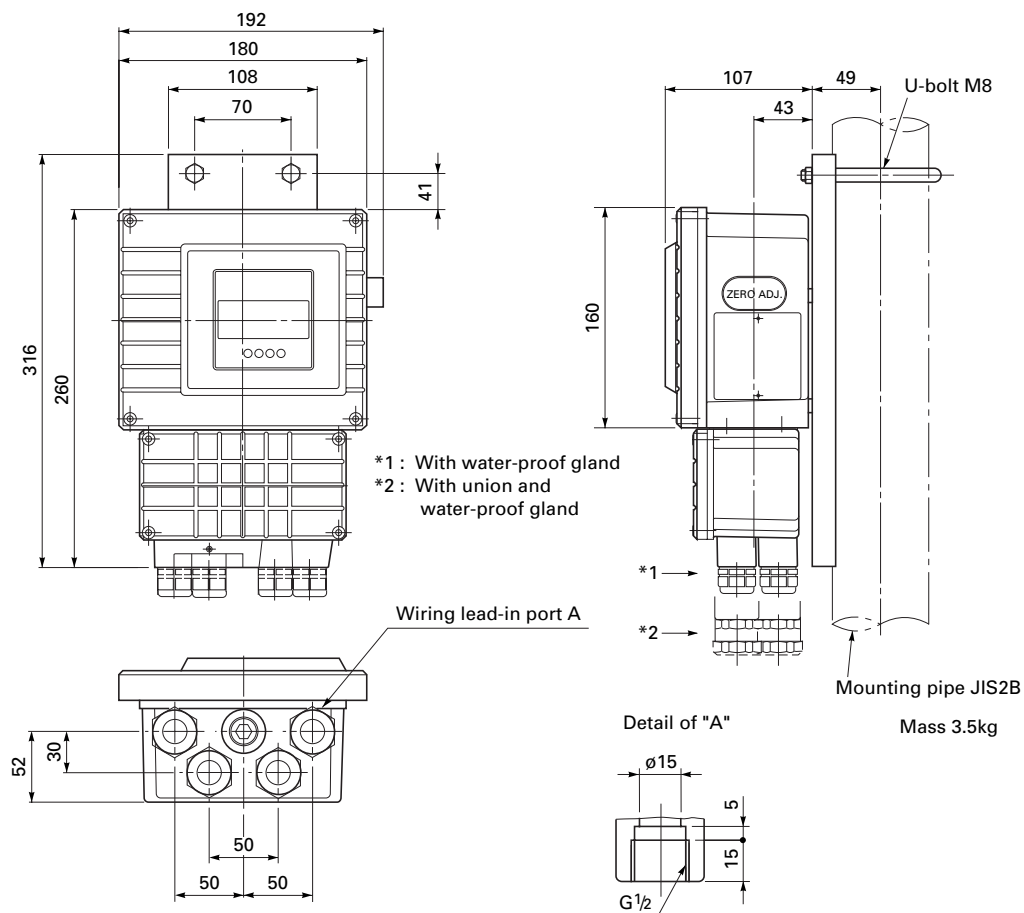


(Wall mount type converter)

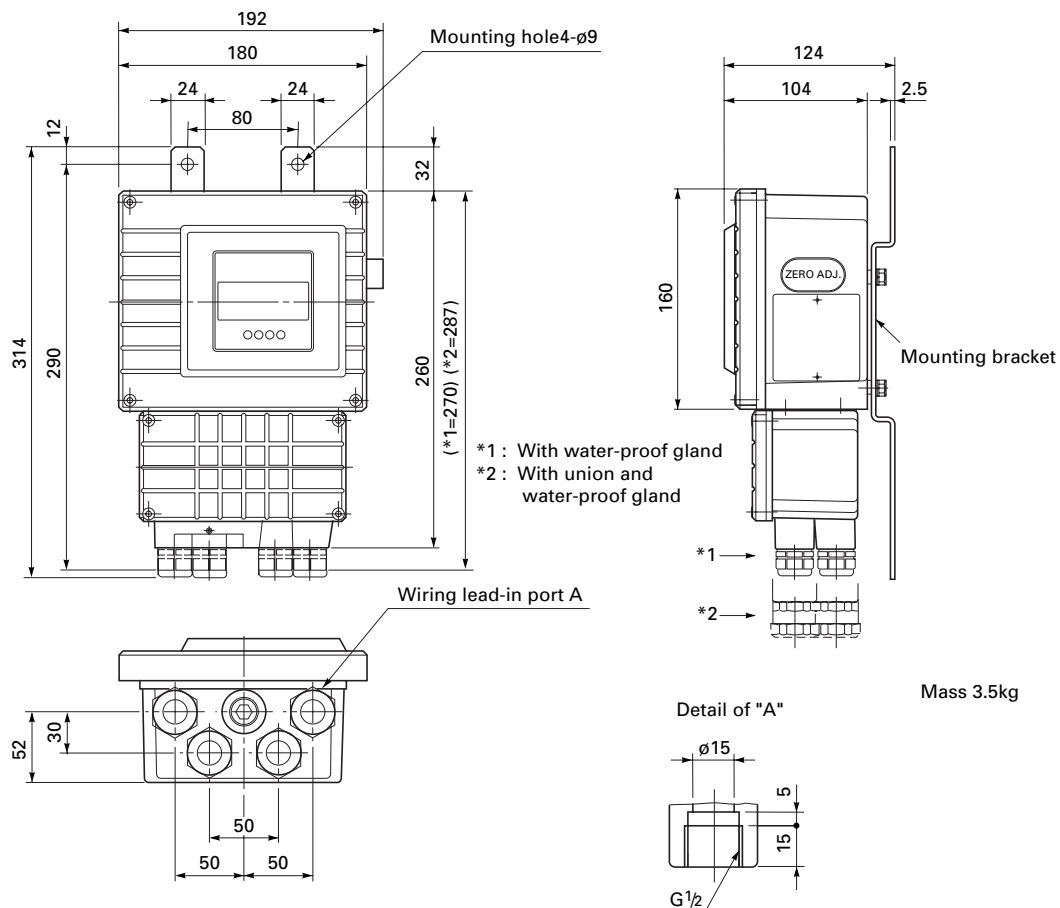

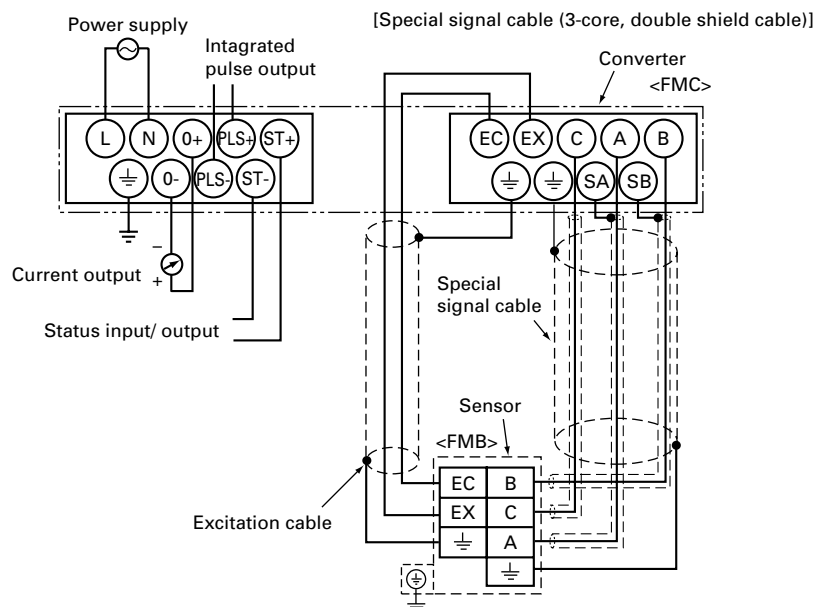

FLOW RATE-FLOW VELOCITY CONVERSION DIAGRAM

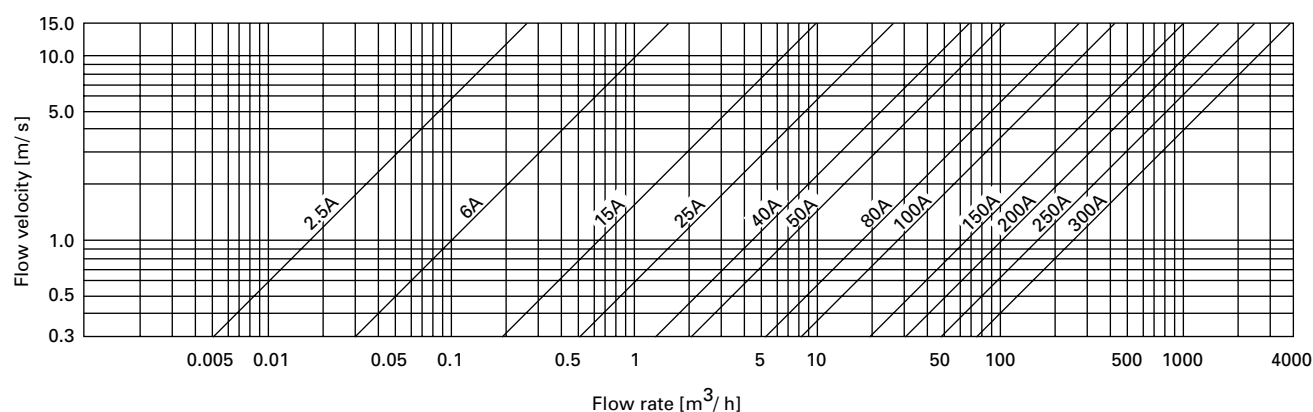

SCOPE OF DELIVERY

Sensor × 1 (mounting bolt and packing should be prepared separately)

Converter × 1 (with pipe mounting or wall mounting bracket)

Special signal cable × 1 (as specified; excitation cable should be prepared separately)

ACCESSORY

- Spare fuse (1A) 1
- Guide rings / for wafer type (Note)
- 1 set spare water-proof gland (for water-proof gland type)

Note) Not supplied for 2.5A-25A ANSI 150LB and 100A, 200A JIS 10K.

ITEMS SPECIFIED AT ORDERING

1. Type, specification code
2. Flow measurement range and measurement fluid
3. Stainless tag plate, and tag No. (less than 16 alphanumeric characters).
4. If you want the instrument with certain parameters factory set as you desire, submit the parameter designation tables 1 and 2 when specifying them.

If you want the instrument with certain parameters factory set as you desire, specify them in parameter designation tables 1 and 2.

Sector : _____

Telephone No. : _____

Measured fluid : _____

Put check marks into ☐ which precede items to modify for.

[illegible]

(Note 1) Standard set value refers to parameter set value as factory set in case parameter setting is not designated.

(Note 2) Designate so that 0.0001 to 1000 pulses integrated will be output per second (so that following expression will hold) when flow rate is maximum.

$$0.0001 \leq \text{range [m}^3/\text{h]} / (\text{integration constant [m}^3] \times 3600) \leq 1000$$

(Note 3) Designate the integrated pulse width so as to hold: (Integration constant [m³]) × 3600/range [m³/h] ≥ integrated pulse width [ms]/500

<Parameter designation table 2>

Setting item	Standard set value (Note 1)	Range	Item to select	Item selection or value designation	Example
Integration low-cut point	3.0%	0.0 to 10.0%	None	— . — [%]	5.0%
Integration burnout	HOLD	HOLD COUNT	<input type="checkbox"/> HOLD <input type="checkbox"/> COUNT	None	
Status function	NO FUNCTION		Select one of functions below.	According to selection on the left, designate item and value.	
		① NO FUNCTION	<input type="checkbox"/> NO FUNCTION	None	
		② External 2 range changeover • 2nd range: 0.1 to 15 m/s converted to flow velocity. • Status input: INPUT CLOSED (Note 4) INPUT OPEN	<input type="checkbox"/> External 2 range changeover	Must be designated in 4 significant digits. 2nd range: — . — . — . — Volume unit: <input type="checkbox"/> mL, <input type="checkbox"/> L, <input type="checkbox"/> m ³ Time unit: <input type="checkbox"/> /s, <input type="checkbox"/> /min, <input type="checkbox"/> /h, <input type="checkbox"/> /d <input type="checkbox"/> INPUT CLOSED <input type="checkbox"/> INPUT OPEN	10.00
		③ External forward/reverse range changeover • 2nd range: 0.1 to 15 m/s converted to flow velocity. • Status input: INPUT CLOSED (Note 4) INPUT OPEN	<input type="checkbox"/> External forward/reverse range changeover	Must be designated in 4 significant digits. 2nd range: — . — . — . — Volume unit: <input type="checkbox"/> mL, <input type="checkbox"/> L, <input type="checkbox"/> m ³ Time unit: <input type="checkbox"/> /s, <input type="checkbox"/> /min, <input type="checkbox"/> /h, <input type="checkbox"/> /d <input type="checkbox"/> INPUT CLOSED <input type="checkbox"/> INPUT OPEN	10.00
		④ 0% signal lock • Status input: INPUT CLOSED (Note 4) INPUT OPEN	<input type="checkbox"/> 0% signal lock	<input type="checkbox"/> INPUT CLOSED <input type="checkbox"/> INPUT OPEN	
		⑤ External zero adjustment • Status input: INPUT CLOSED (Note 4) INPUT OPEN	<input type="checkbox"/> External zero adjustment	<input type="checkbox"/> INPUT CLOSED <input type="checkbox"/> INPUT OPEN	
		⑥ External integration preset • Status input: INPUT CLOSED (Note 4) INPUT OPEN * Designate preset value separately in item of “integration preset value”.	<input type="checkbox"/> External integration preset	<input type="checkbox"/> INPUT CLOSED <input type="checkbox"/> INPUT OPEN	
		⑦ Automatic 2 range changeover • 2nd range: 0.1 to 15 m/s converted to flow velocity. • Changeover hysteresis: 0.0 to 20.0% (with respect to smaller range). • Status output: OUTPUT ON (Note 5) OUTPUT OFF	<input type="checkbox"/> Automatic 2 range changeover	Must be designated in 4 significant digits. 2nd range: — . — . — . — Volume unit: <input type="checkbox"/> mL, <input type="checkbox"/> L, <input type="checkbox"/> m ³ Time unit: <input type="checkbox"/> /s, <input type="checkbox"/> /min, <input type="checkbox"/> /h, <input type="checkbox"/> /d Hysteresis: — . — . — . — % <input type="checkbox"/> OUTPUT ON <input type="checkbox"/> OUTPUT OFF	10.00 5.0%
		⑧ Automatic forward/reverse changeover • 2nd range: 0.1 to 15 m/s converted to flow velocity. • Changeover hysteresis: 0.0 to 10.0% (with respect to smaller range). • Status output: OUTPUT ON (Note 5) OUTPUT OFF	<input type="checkbox"/> Automatic forward/reverse changeover	Must be designated in 4 significant digits. 2nd range: — . — . — . — Volume unit: <input type="checkbox"/> mL, <input type="checkbox"/> L, <input type="checkbox"/> m ³ Time unit: <input type="checkbox"/> /s, <input type="checkbox"/> /min, <input type="checkbox"/> /h, <input type="checkbox"/> /d Hysteresis: — . — . — . — % <input type="checkbox"/> OUTPUT ON <input type="checkbox"/> OUTPUT OFF	10.00 5.0%
		⑨ Flow switch • Upper limit: -10.0 to 110.1% (if 110.1% is selected, upper limit is invalid). • Lower limit: -10.1 to 110.0% (if -10.1% is selected, lower limit is invalid). • Status output: OUTPUT ON (Note 5) OUTPUT OFF	<input type="checkbox"/> Flow switch	Upper limit: — . — . — . — [%] Lower limit: — . — . — . — [%] <input type="checkbox"/> OUTPUT ON <input type="checkbox"/> OUTPUT OFF	+90.0[%] -02.0[%]
		⑩ Integration switch • Set value: -9999999999 to +9999999999 • Status output: OUTPUT ON (Note 5) OUTPUT OFF * Unit is the same as set value for integration constant.	<input type="checkbox"/> Integration switch	Set value: — . — . — . — . — . — . — . — <input type="checkbox"/> OUTPUT ON <input type="checkbox"/> OUTPUT OFF	
		⑪ Alarm output • Alarm selection ALL FUNCTION, HARDWARE FAULT, PROCESS FAULT • Status output: OUTPUT ON (Note 5) OUTPUT OFF	<input type="checkbox"/> Alarm output	• Alarm selection <input type="checkbox"/> ALL FUNCTION <input type="checkbox"/> HARDWARE FAULT <input type="checkbox"/> PROCESS FAULT • Status output: <input type="checkbox"/> OUTPUT ON <input type="checkbox"/> OUTPUT OFF	
Empty detection function	INHIBIT	INHIBIT ENABLE	<input type="checkbox"/> INHIBIT <input type="checkbox"/> ENABLE	None	
TAG-NO	Blank unless designated	Up to 16 alphanumerics	None	— . — . — . — . — . — . — . — — . — . — . — . — . — . — . —	F-100
Flow direction	FORWARD	FORWARD REVERSE	<input type="checkbox"/> FORWARD <input type="checkbox"/> REVERSE	None	

(Note 4) Status input specifications: No-voltage contact. 1 kΩ or less when closed. 50 kΩ or more when open.

(Note 5) Status output specifications: Capacity; 30V DC or less, 0.2A or less, ON voltage; 2V or less

⚠ Caution on Safety

*Before using this product, be sure to read its instruction manual in advance.

Fuji Electric Systems Co., Ltd.

Head Office

Gate City Ohsaki, East Tower, 11-2, Osaki 1-chome,
Shinagawa-ku, Tokyo 141-0032, Japan
<http://www.fesys.co.jp/eng>

Instrumentation Div. International Sales Dept.

No.1, Fuji-machi, Hino-city, Tokyo, 191-8502 Japan
Phone: 81-42-585-6201, 6202 Fax: 81-42-585-6187
<http://www.fic-net.jp/eng>

Information in this catalog is subject to change without notice.

Printed in Japan