

# Mini-spectrometer

[ FT series ]

C13054MA



**Compact and thin,  
built-in high-sensitivity CMOS image sensor for  
Raman spectroscopy**

The mini-spectrometer FT (flat type) series is a polychromator provided in a compact, thin case that houses optical elements, image sensor, and driver circuit. Spectrum data can be acquired by guiding measurement light into a mini-spectrometer through an optical fiber and transferring the measured results to a PC via the USB connection. The incorporation of a high-sensitivity CMOS image sensor maintains high sensitivity equivalent to that of a CCD and achieves low power consumption. Moreover, the trigger function that can be used for short-term integration enables spectroscopic measurement of pulse emissions.

The product includes evaluation software with functions for setting measurement conditions, acquiring and saving data, drawing graphs, and so on. Furthermore, the DLL function specifications are disclosed, so users can create their original measurement software programs.

## Features

- **Compact, thin case**
- **Highly accurate optical characteristics: High spectral resolution 0.4 nm**
- **High-sensitivity CMOS image sensor built in (high sensitivity equivalent to that of a CCD)**
- **With trigger function**
- **High throughput using quartz transmission grating**
- **External power supply not necessary (USB bus powered)**
- **Easy installation in devices**
- **Stores wavelength conversion factor\*1 in internal memory**

\*1: A conversion factor for converting the image sensor pixel number into a wavelength. A calculation factor for converting the A/D converted count into the input light level is not provided.

## Applications

- **Raman spectroscopy**

## Optical characteristics

Parameter	Specification	Unit
Spectral response range	790 to 920	nm
Spectral resolution (FWHM)*2	Typ.	0.4
	Max.	0.7
Wavelength reproducibility*3	-0.2 to +0.2	nm
Wavelength temperature dependence	-0.02 to +0.02	nm/°C
Spectral stray light*2 *4	-33 max.	dB

\*2: When the slit in the table in "Structure" is used. The spectral resolution depends on the slit.

\*3: Measured under constant light input conditions

\*4: The ratio of the count measured when an 860 nm light is input to the count measured when an 860 ± 10 nm light is input

## Electrical characteristics

Parameter	Specification	Unit
A/D conversion	16	bit
Integration time	11 to 100000	μs
Interface	USB 2.0	-
USB bus power current consumption	Typ.	220
	Max.	250

## Structure

Parameter	Specification	Unit
Dimensions (W × D × H)	80 × 60 × 12	mm
Weight	88	g
Image sensor	High-sensitivity CMOS linear image sensor	-
Number of pixels	512	pixels
Slit*5 (H × V)	10 × 400	μm
NA*6	0.11	-
Connector for optical fiber	SMA905	-

\*5: Input slit aperture size

\*6: Numeric aperture (solid angle)

## Absolute maximum ratings


Parameter	Value	Unit
Operating temperature*7	+5 to +40	°C
Storage temperature*7	-20 to +70	°C

\*7: No dew condensation


When there is a temperature difference between a product and the surrounding area in high humidity environment, dew condensation may occur on the product surface. Dew condensation on the product may cause deterioration in characteristics and reliability.

Note: Exceeding the absolute maximum ratings even momentarily may cause a drop in product quality. Always be sure to use the product within the absolute maximum ratings.


## Spectral response (typical example)

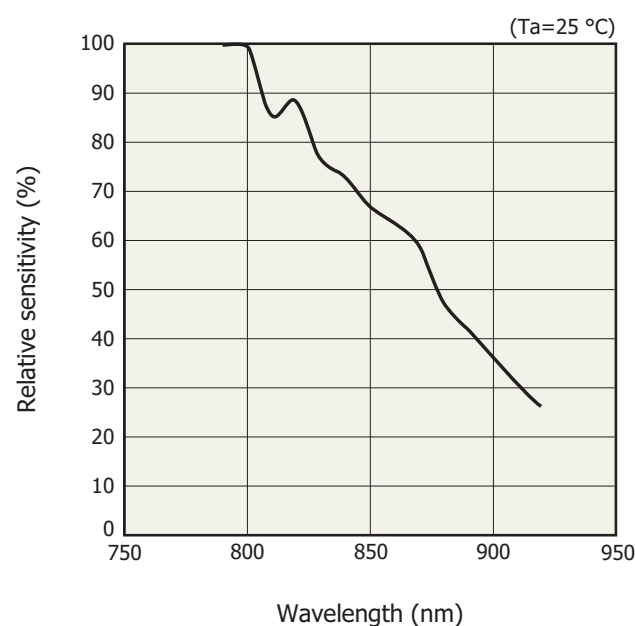

## Spectral resolution vs. wavelength (typical example)

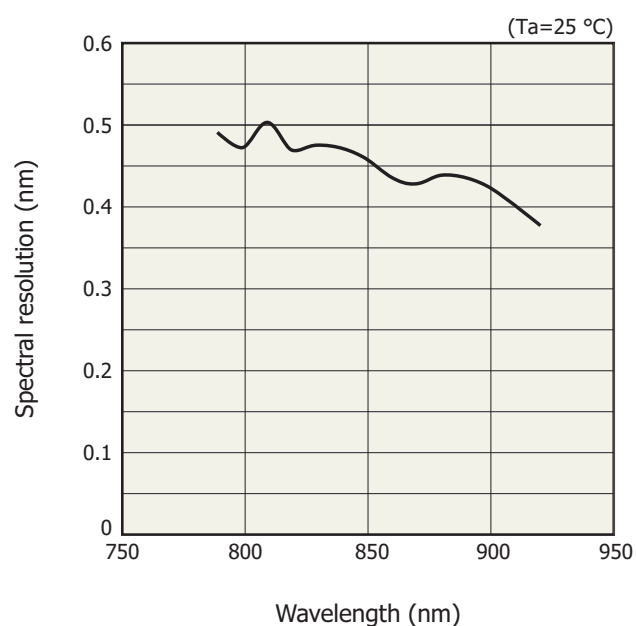


### Linearity (typical example)

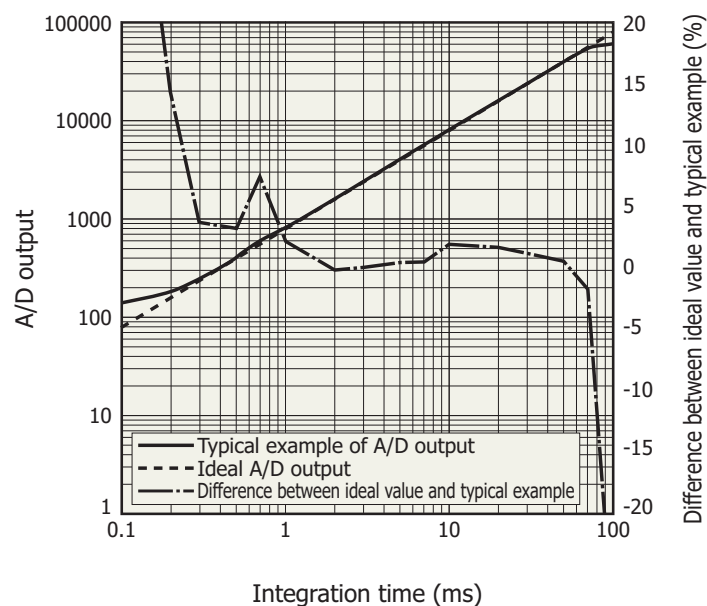

KACCB0380EA

A/D output is the output with dark output is subtracted when light is input. The difference between the ideal value and typical example contains a measurement error. The smaller the A/D output, the larger the measurement error.

### Dark output vs. temperature (typical example)

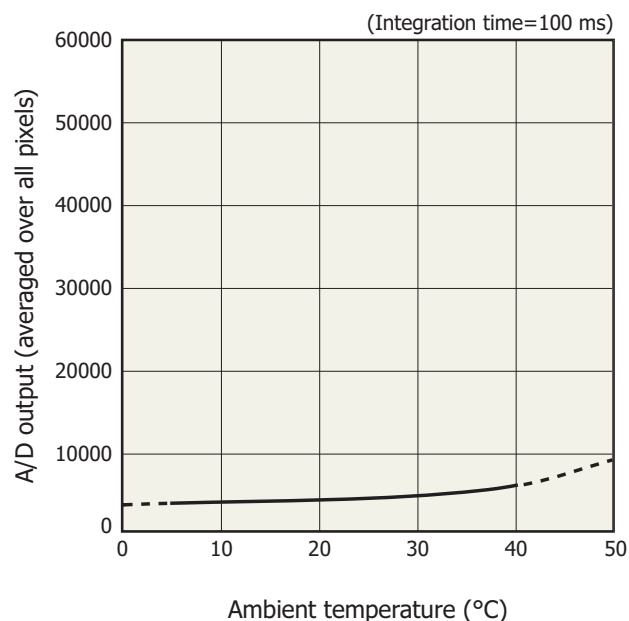


KACCB0370EA

A/D output is the sum of the sensor and circuit offset outputs and the sensor dark output.

### Optical component layout


The mini-spectrometer FT series employs a transmission holographic grating made of quartz and an optical system arranged on a robust optical base to produce high throughput and highly accurate optical characteristics.

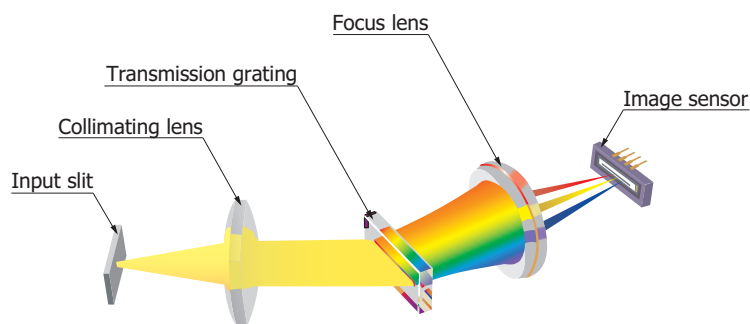

KACCC0256EA

## Connection example (transmitted light measurement)

Spectrum data can be acquired by guiding measurement light into a mini-spectrometer through an optical fiber and transferring the measured results to a PC via the USB connection. Since there are no moving parts inside the device, constantly stable measurements can be expected. Moreover, the optical guiding section uses an optical fiber making connection to the measured object flexible.

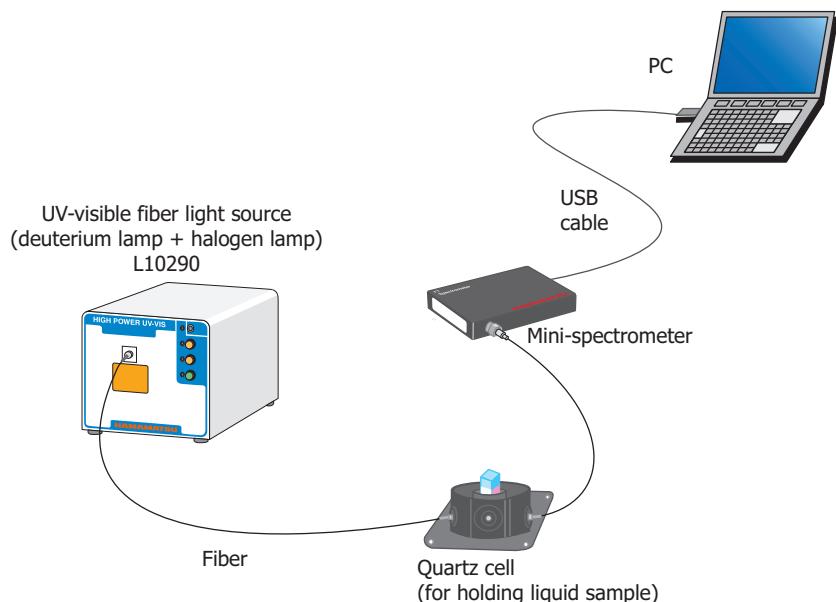


KACCC0790EA

## Trigger operation modes

In the C13054MA, the following trigger operation modes are available. You can switch between these modes from the evaluation software supplied with the C13054MA.

### (1) Asynchronous data measurement at software trigger input


The first piece of digital data that is converted after a software trigger is applied from the PC is acquired.

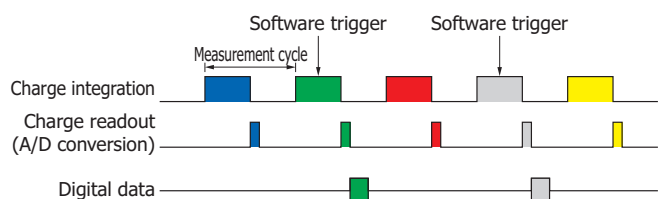

KACCC0503EC

### (2) Synchronous data measurement at software trigger input


Sensor operation (integration) starts when a software trigger is applied from the PC.

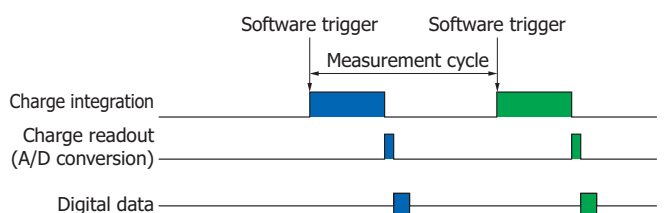

KACCC0505EB


## (3) Asynchronous data measurement at external trigger input

The first piece of digital data that is converted after an external trigger edge (rising or falling edge can be specified) is applied to the external trigger terminal is acquired.

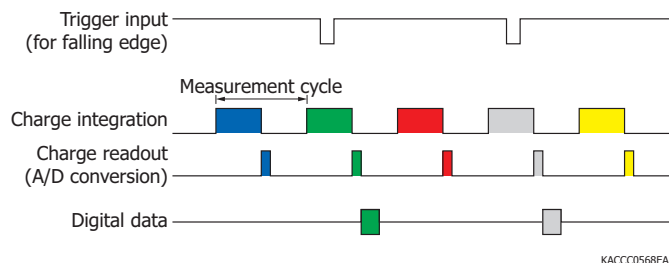


## (4) Synchronous data measurement at external trigger input

Sensor operation (integration) starts when an external trigger edge (rising or falling edge can be specified) is applied to the external trigger terminal, and then the digital data is acquired.

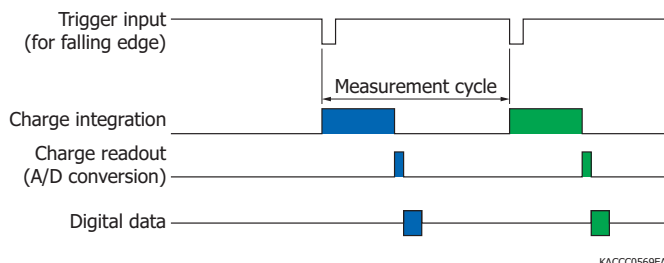


## (5) Asynchronous data measurement at external trigger input level

Digital data is acquired when an external trigger (high level or low level can be specified) is applied to the external trigger terminal.

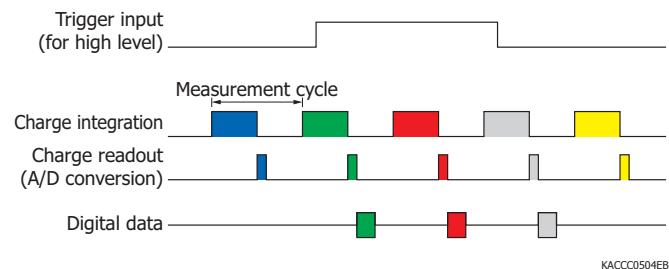

## (6) Synchronous data measurement at external trigger input level


Sensor operation (integration) starts when a trigger (high level or low level can be specified) is applied to the external trigger terminal, and then the digital data is acquired.

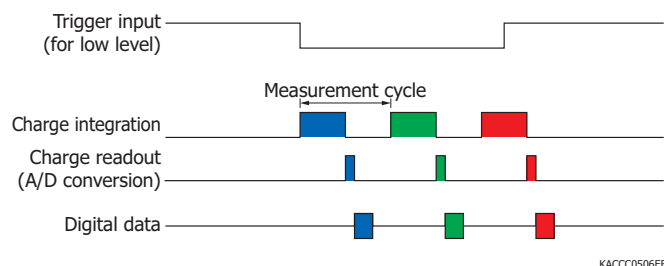

In any of the modes (1) to (6), if the trigger input cycle is shorter than the measurement cycle of the spectrometer, the input trigger is ignored.

## (7) External trigger signal output


The start timing (pulse width: 10  $\mu$ s) of integration can be output from the external trigger terminal (trigger output edge: rising or falling edge can be specified).

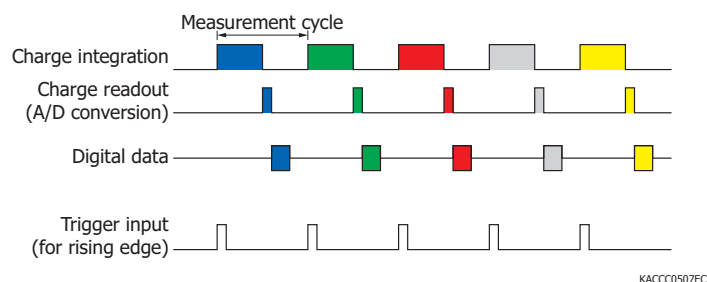

### Evaluation software (accessory)

By installing the evaluation software (SpecEvaluationUSB2.exe)\*8 into a PC, you can perform the following basic operations.

- Acquire and save measured data
- Set measurement conditions
- Module information acquisition (wavelength conversion factor, mini-spectrometer type, etc.)
- Display graphs
- Arithmetic functions
  - Pixel number to wavelength conversion
  - Calculation in comparison with reference data (transmittance, reflectance)
  - Dark subtraction
  - Gaussian approximation (peak position and count, FWHM)

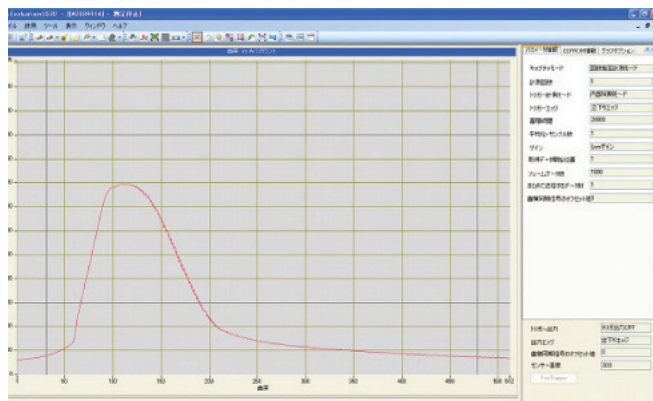

Note: Up to eight mini-spectrometers can be connected to a single PC and used.

#### \*8: Compatible OS

- Microsoft® Windows® 7 Professional SP1 (32-bit, 64-bit)
- Microsoft® Windows® 8 Professional (32-bit, 64-bit)


A DLL for controlling the hardware is available.

Users can develop original measurement programs using the following development platform.

- Microsoft® Visual Studio® 2008 (SP1) Visual C++®
- Microsoft® Visual Studio® 2008 (SP1) Visual Basic®

Note: Microsoft, Windows, Visual Studio, Visual C++, and Visual Basic are either registered trademarks or trademarks of Microsoft Corporation in the United States and/or other countries.

### Dimensional outline (unit: mm)

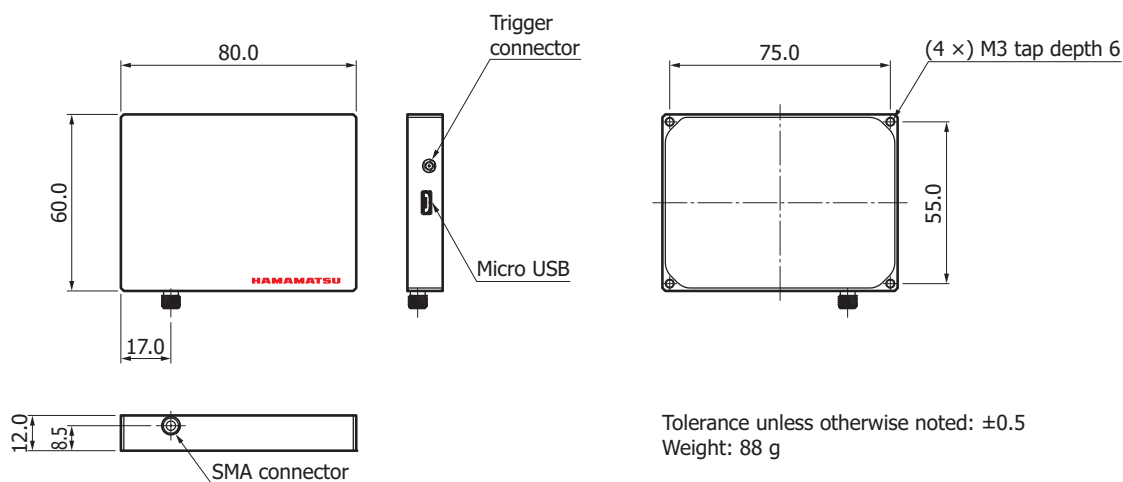

Tolerance unless otherwise noted:  $\pm 0.5$   
Weight: 88 g

KACCA0364EA

## Accessories

- USB cable
- Dedicated software (evaluation software, sample software, DLL)


## Options (sold separately)

- Input optical fiber

Type no.	Product name	Core diameter (μm)	Specification
A9762-01	Fiber for visible/near infrared range	600	NA=0.22, length=1.5 m, low cost With SMA905D connector on each end
A9763-05		400	NA=0.22, length=1.5 m, small bending radius at fiber section With SMA905D connector on each end

- External trigger input coaxial cable A12763

Dimensional outline (unit: mm)

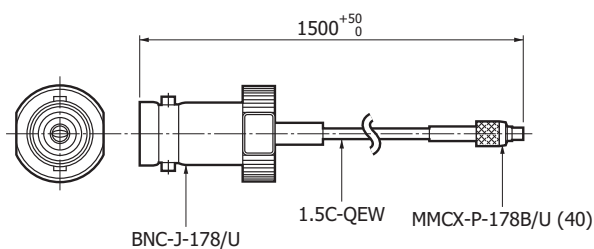

KACCA0358EA

## Mini-spectrometer lineup

Type no.	Type		Spectral response range (nm)														Spectral resolution max. (nm)	Image sensor	
			200	400	600	800	1000	1200	1400	1600	1800	2000	2200	2400	2600				
C10082CA	Mini-spectrometer TM series	TM-UV/VIS-CCD High sensitivity																6	Back-thinned CCD image sensor
C10082CAH		TM-UV/VIS-CCD High resolution		200 to 800													1*		
C10082MD		TM-UV/VIS-MOS Wide dynamic range																6	CMOS linear image sensor
C10083CA		TM-VIS/NIR-CCD High sensitivity																8 (λ=320 to 900 nm)	Back-thinned CCD image sensor
C10083CAH		TM-VIS/NIR-CCD High resolution																1* (λ=320 to 900 nm)	
C10083MD		TM-VIS/NIR-MOS Wide dynamic range			320 to 1000													8	CMOS linear image sensor
C11697MB		TM-VIS/NIR-MOS-II Trigger-compatible																8	High-sensitivity CMOS linear image sensor
C9404CA	Mini-spectrometer TG series	TG-UV-CCD High sensitivity		200 to 400														3	Back-thinned CCD image sensor
C9404CAH		TG-UV-CCD High resolution																1*	
C9405CB		TG-SWNIR-CCD-II IR-enhanced				500 to 1100												5 (λ=550 to 900 nm)	IR-enhanced back-thinned CCD image sensor
C11713CA		TG-RAMAN-I High resolution				500 to 600													0.3*
C11714CB	TG-RAMAN-II High resolution						790 to 920											0.3*	IR-enhanced back-thinned CCD image sensor
C11482GA	Mini-spectrometer TG series	TG2-NIR Non-cooled type					900 to 1700											7	InGaAs linear image sensor
C9913GC		TG-cooled NIR-I Low noise (cooled type)																7	
C9914GB		TG-cooled NIR-II Low noise (cooled type)						1100 to 2200										8	
C11118GA		TG-cooled NIR-III Low noise (cooled type)						900 to 2550											
C13053MA	Mini-spectrometer FT series	FT-SWIR-MOS-II Compact, thin case			500 to 1100													3.5	High-sensitivity CMOS linear image sensor
C13054MA		FT2-RAMAN Compact, thin case						790 to 920										0.4*	
C11007MA	Mini-spectrometer RC series	RC-VIS-MOS Spectrometer module		340 to 780														9	CMOS linear image sensor
C11008MA		RC-SWNIR-MOS Spectrometer module				640 to 1050												8	IR-enhanced CMOS linear image sensor

\* Typ.

For installation into mobile measuring equipment

Type no.	Type		Spectral response range (nm)														Spectral resolution max. (nm)	Image sensor
			200	400	600	800	1000	1200	1400	1600	1800	2000	2200	2400	2600			
C11009MA	Mini-spectrometer RC series	RC-VIS-MOS Spectrometer head			340 to 780												9	CMOS linear image sensor
C11010MA		RC-SWNIR-MOS Spectrometer head				640 to 1050												8

For installation into mobile measuring equipment (ultra-compact)

Type no.	Type		Spectral response range (nm)														Spectral resolution max. (nm)	Image sensor
			200	400	600	800	1000	1200	1400	1600	1800	2000	2200	2400	2600			
C11708MA	Mini-spectrometer MS series	MS-SWNIR-MOS Spectrometer head				640 to 1050										20	CMOS linear image sensor	
C12666MA		Spectrometer head		340 to 780												15	CMOS linear image sensor	
C12880MA	Micro-spectrometer	Spectrometer head		340 to 850												15	High-sensitivity CMOS linear image sensor	



## Related information

[www.hamamatsu.com/sp/ssd/doc\\_en.html](http://www.hamamatsu.com/sp/ssd/doc_en.html)

### ■ Precautions

- Disclaimer
- Mini-spectrometers

### ■ Technical information

- Mini-spectrometers

Information described in this material is current as of October, 2015.

Product specifications are subject to change without prior notice due to improvements or other reasons. This document has been carefully prepared and the information contained is believed to be accurate. In rare cases, however, there may be inaccuracies such as text errors. Before using these products, always contact us for the delivery specification sheet to check the latest specifications.

The product warranty is valid for one year after delivery and is limited to product repair or replacement for defects discovered and reported to us within that one year period. However, even if within the warranty period we accept absolutely no liability for any loss caused by natural disasters or improper product use. Copying or reprinting the contents described in this material in whole or in part is prohibited without our prior permission.

# HAMAMATSU

[www.hamamatsu.com](http://www.hamamatsu.com)

HAMAMATSU PHOTONICS K.K., Solid State Division

1126-1 Ichino-cho, Higashi-ku, Hamamatsu City, 435-8558 Japan, Telephone: (81) 53-434-3311, Fax: (81) 53-434-5184

U.S.A.: Hamamatsu Corporation: 360 Foothill Road, Bridgewater, N.J. 08807, U.S.A., Telephone: (1) 908-231-0960, Fax: (1) 908-231-1218

Germany: Hamamatsu Photonics Deutschland GmbH: Arzbergerstr. 10, D-82211 Herrsching am Ammersee, Germany, Telephone: (49) 8152-375-0, Fax: (49) 8152-265-8

France: Hamamatsu Photonics France S.A.R.L.: 19, Rue du Saule Trapu, Parc du Moulin de Massy, 91882 Massy Cedex, France, Telephone: 33-(1) 69 53 71 00, Fax: 33-(1) 69 53 71 10

United Kingdom: Hamamatsu Photonics UK Limited: 2 Howard Court, 10 Tewin Road, Welwyn Garden City, Hertfordshire AL7 1BW, United Kingdom, Telephone: (44) 1707-294888, Fax: (44) 1707-325777

North Europe: Hamamatsu Photonics Norden AB: Torshamnsgatan 35 16440 Kista, Sweden, Telephone: (46) 8-509-031-00, Fax: (46) 8-509-031-01

Italy: Hamamatsu Photonics Italia S.r.l.: Strada della Moia, 1 int. 6, 20020 Arese (Milano), Italy, Telephone: (39) 02-93581733, Fax: (39) 02-93581741

China: Hamamatsu Photonics (China) Co., Ltd.: B1201, Jiaming Center, No.27 Dongsanhuan Beilu, Chaoyang District, Beijing 100020, China, Telephone: (86) 10-6586-6006, Fax: (86) 10-6586-2866